

# Advanced Electron Density Phantom

## Tissue-Equivalent CT-to-Electron Density Calibration

- Meets medical standards for human tissue mimicking materials: ICRU-44 and ICRP
- Expanded phantom size for wide (CBCT and Fan) beam systems
- CT-to-density table automation with patented rod markers and RapidCHECK™ software
- Compatible with any ion chamber




Accurately converting CT values to HU or electron density values plays an important role in transitioning from diagnosis to a specific treatment protocol. With the Advanced Electron Density Phantom, ICRU-44 matched tissue equivalence, automation and smart design all serve to remove uncertainties from your energy conversions.

Our materials are manufactured to meet medical standards for human tissue densities.

### Workflow Automation with RapidCHECK™


Our patented rod markers uniquely identify each material during the CT scan. This enables automated CT-to-density analysis, saving valuable time and reducing risk of error. Using RapidCHECK™ software to automatically find and identify the material of each rod streamlines the CT-to-electron density calibration.

Get results immediately. Load data. Get analysis. Print a report. Track changes over time. If issues are detected, easily review prior scans, analyze trends, and investigate anomalous results.

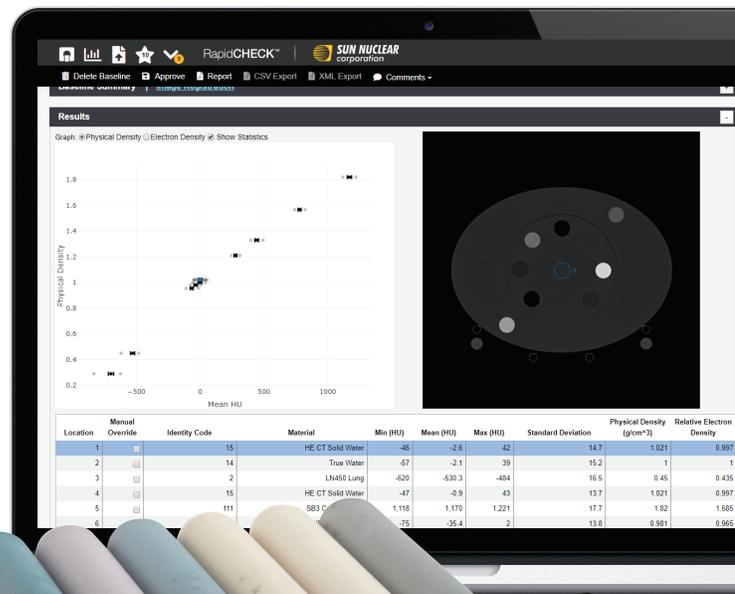

## Features and Benefits

- Expanded Size
  - Extends 16.5 cm in the superior/inferior direction
  - Full-length 16.5 cm rods, not just 5 cm
  - Oblate-shaped, 40 cm wide by 30 cm high
  - Removable 20 cm head section
  - Increases to 26.5 cm in length with optional extension plates
- Proven Gammex® Technologies
  - Constructed from zero HU CT Solid Water® HE
  - Tissue Mimicking Materials developed in accordance with ICRU-44 and ICRP specifications
- Automation
  - Patented rod markers uniquely identify each material in a CT scan
  - Automatically generate CT-to-density tables with RapidCHECK™ software support
  - Rod markers remove risk of misplaced rods, rotated phantoms, and incorrect selection of ROIs
- Ease of Use
  - Single-pour, no-drop design simplifies transport and setup
  - Self-aligning rods and sections lie flush for fast and reliable positioning
  - Custom wheeled case and deluxe stand included
  - Compatible with any ion chamber. Upon ordering specify which ion chamber you intend to use.

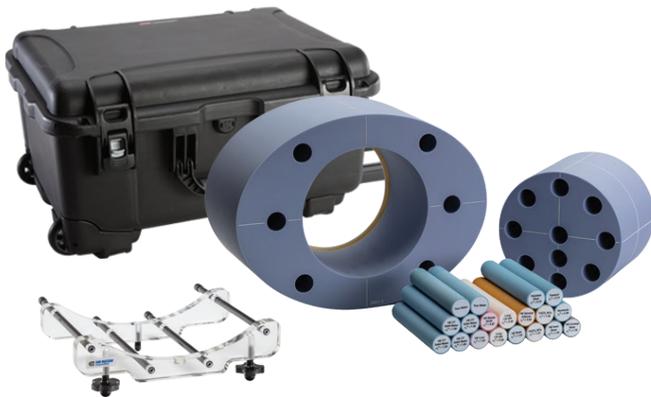


## Specifications

In-plane Dimensions:	40.0 cm (15.7 in) x 30.0 cm (11.8 in)
Depth:	16.5 cm (6.3 in), up to 26.5 cm (10.2 in) with optional extension plates
Diameter of Removable Head Section:	20.0 cm (7.87 in)
Material:	HE Energy-Matched CT Solid Water®
Interchangeable Inserts:	14 solid inserts plus 2 true water containers
Optional inserts include:	Aluminum, Stainless Steel, Titanium
Optional Accessories:	Extension plates Ion Chamber conversion rod
Weight:	15.5 kg (34.1 lbs)
Case:	Wheeled case is included
Stand:	Stand is included

## Standard Inserts

Material	Physical Density (g/cm <sup>3</sup> )	Electron Density Relative to Water
455 Lung LN-300	0.29	0.28
485 Lung LN-450	0.45	0.44
1553 HE Gen Adipose	0.96	0.94
1454 HE Breast 50:50	0.98	0.97
4 - 1451 HE CT Solid Water® Inserts	1.02	1.00
1481 HE Brain	1.05	1.02
1482 HE Liver	1.08	1.05
1456 HE Inner Bone	1.21	1.16
484 CB2 + 30% CaCO <sub>3</sub>	1.33	1.27
480 CB2 + 50% CaCO <sub>3</sub>	1.56	1.46
1450 HE Cortical Bone	1.93	1.78
2 - True Water Inserts	-1.000-	-1.000-

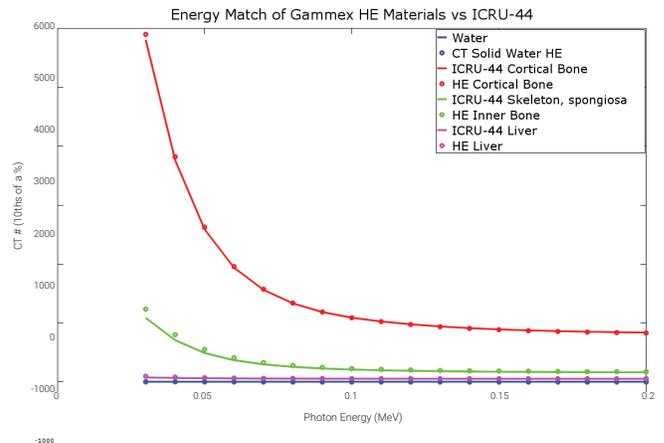

Gammex materials match the density characteristics of ICRU-44 materials **AND** their energy dependencies.

<sup>1</sup> American Association of Physicists in Medicine Radiation Therapy Committee Task Group 53: Quality Assurance for Clinical Radiotherapy Treatment Planning

<sup>2</sup> IAEA TECDOC-1583. Commissioning of Radiotherapy Treatment Planning Systems: Testing for Typical External Beam Treatment Techniques